



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11) **EP 1 295 570 A2**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
26.03.2003 Bulletin 2003/13

(51) Int Cl.7: **A61F 2/00**

(21) Application number: **02018239.0**

(22) Date of filing: **21.08.2002**

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
IE IT LI LU MC NL PT SE SK TR**
Designated Extension States:
AL LT LV MK RO SI

(72) Inventors:
• **Schwager, Michael**
8404 Winterthur (CH)
• **Frei, Martin**
8200 Schaffhausen (CH)
• **Ha, Suk-Woo**
8246 Langwiesen (CH)

(30) Priority: **19.09.2001 US 957216**

(71) Applicant: **JOMED GmbH**
72414 Rangendingen (DE)

(74) Representative: **VOSSIUS & PARTNER**
Siebertstrasse 4
81675 München (DE)

(54) **Cold-molding process for loading a stent onto a stent delivery system**

(57) A method of making a stent delivery system is provided in which a delivery catheter has a balloon that extends non-uniformly into interstices of a stent. In accordance with the method a balloon/stent/crimping tube assembly is placed in a crimping tool, the balloon is inflated, and the crimping tool is actuated to compress the stent on the outside of the balloon without application of

heat or chemicals, thereby causing creases of the balloon to extend non-uniformly into the interstices of the stent. Optionally, pillows may be formed in the balloon to prevent longitudinal movement of the stent with respect to the balloon during intravascular delivery. One or more secondary crimpings also may be performed to achieve a smoother delivery profile.

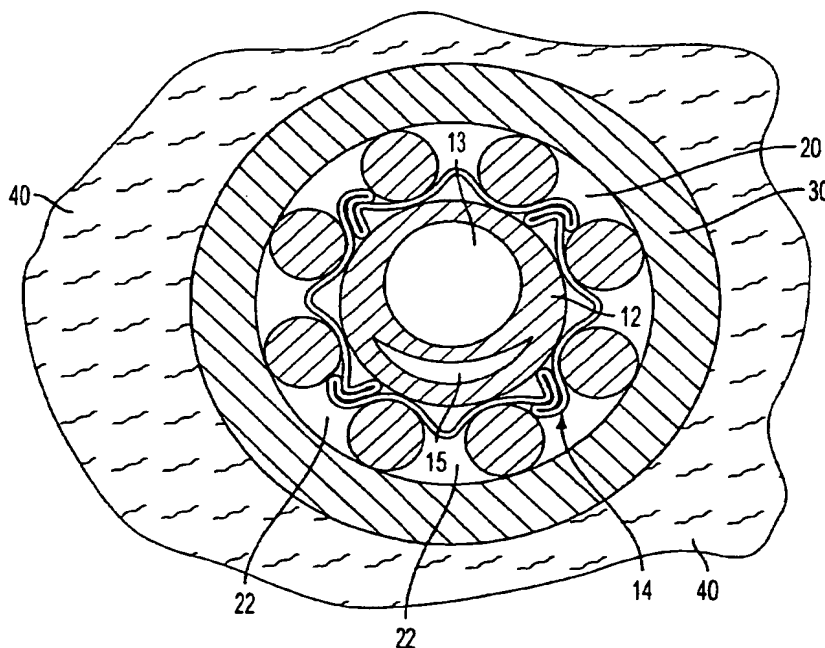


FIG. 5A

Description

[0001] The present invention relates to a cold-molding process for loading a stent onto a stent delivery system. More specifically, the present invention relates to a method of loading a stent onto a balloon having creases that extend non-uniformly into the interstices of the stent without the use of a heating step.

[0002] A stent is commonly used alone or in conjunction with angioplasty to ensure patency through a patient's stenosed vessel. Stents overcome the natural tendency of the vessel walls of some patients to restenose after angioplasty. A stent is typically inserted into a vessel, positioned across a lesion, and then expanded to create or maintain a passageway through the vessel, thereby restoring near-normal blood flow through the vessel.

[0003] A variety of stents are known in the art, including self-expandable and expandable stents, as well as wire braid stents. One such stent is described, for example, in U.S. Patent No. 4,733,665 to Palmaz. Expandable stents are typically delivered to treatment sites on delivery devices, such as balloon catheters or other expandable devices. Balloon catheters may comprise a balloon having a collapsed delivery configuration with wings that are wrapped and folded about the catheter. An expandable stent is then disposed in a collapsed delivery configuration about the balloon by compressing the stent onto the balloon. The stent and balloon assembly may then be delivered, using well-known percutaneous techniques, to a treatment site within the patient's vasculature, for example, within the patient's coronary arteries. Once the stent is positioned across a lesion at the treatment site, it is expanded to a deployed configuration by inflating the balloon. The stent contacts the vessel wall and maintains a path for blood flow through the vessel.

[0004] Significant difficulties have been encountered during stent delivery and deployment, including difficulty in maintaining the stent on the balloon and in achieving symmetrical expansion of the stent when deployed. Several techniques have been developed to more securely anchor the stent to the balloon and to ensure more symmetrical expansion. These include plastically deforming the stent so that it is crimped onto the balloon, and sizing the stent such that its internal diameter provides an interference fit with the outside diameter of the balloon catheter. Such techniques have several drawbacks, including less than optimal securement of the stent to the balloon. Consequently, the stent may become prematurely dislodged from the balloon during advancement of the stent delivery system to the treatment site.

[0005] Stent delivery systems utilizing a removable sheath disposed over the exterior surface of the stent, which is removed once the stent is positioned at the treatment site, have also been proposed, for example, in U.S. Patent No. 5,690,644 to Yurek et al. Such systems

may be used with or without retainer rings and are intended to protect the stent during delivery and to provide a smooth surface for easier passage through the patient's vasculature. However, the exterior sheath increases the crossing profile of the delivery system while decreasing flexibility, thereby decreasing the ability of the device to track through narrowed and tortuous anatomy.

[0006] U.S. Patent No. 6,106,530 to Harada describes a stent delivery device comprising a balloon catheter having stoppers disposed proximal and distal of a balloon on to which a stent is affixed for delivery. The stoppers are separate from the balloon and maintain the stent's position in relation to the balloon during delivery. As with the removable sheaths discussed previously, the stoppers are expected to increase delivery profile and decrease flexibility of the stent/balloon system.

[0007] U.S. Patent No. 6,110,180 to Foreman et al. provides a catheter with a balloon having pre-formed, outwardly-extending protrusions on the exterior of the balloon. A stent may be crimped onto the balloon such that the protrusions extend into the gaps of the stent, thereby securing the stent about the balloon for delivery. A drawback to this device is the added complexity involved in manufacturing a balloon with pre-formed protrusions. Additionally, if the protrusions are not formed integrally with the balloon, there is a risk that one or more of the protrusions may detach during deployment of the stent. The protrusions may also reduce flexibility in the delivery configuration, thereby reducing ability to track through tortuous anatomy.

[0008] U.S. Patent No. 5,836,965 to Jendersee et al. describes a hot-molding process for encapsulating a stent on a delivery system. Encapsulation entails placement of the stent over a balloon, placement of a sheath over the stent on the balloon, and heating the pressurized balloon to cause it to expand around the stent within the sheath. The assembly is then cooled while under pressure to cause the balloon to adhere to the stent and to set the shape of the expanded balloon, thereby providing substantially uniform contact between the balloon and the stent. This method also provides a substantially uniform delivery profile along the surface of the encapsulated balloon/stent assembly.

[0009] A significant drawback of Jendersee's encapsulation method is the need to heat the balloon in order to achieve encapsulation. Such heating while under pressure may lead to localized plastic flows resulting in inhomogeneities along the length of the balloon including, for example, varying wall thickness. Varying wall thickness may, in turn, yield areas of decreased strength that are susceptible to rupture upon inflation of the balloon during deployment of the stent. Additionally, heating and cooling increases the complexity, time, and cost associated with affixing the stent to the balloon.

[0010] U.S. Patent No. 5,976,181 to Whelan et al. provides an alternative technique for stent fixation involving

the use of solvents to soften the balloon material. In this method, the stent is disposed over an evacuated and wrapped balloon while in its compact delivery configuration. A rigid tube is then placed over the stent and balloon assembly, and the balloon is pressurized while the balloon is softened by application of a solvent and/or heating. The rigid tube prevents the stent from expanding but allows the balloon to deform so that its surface projects through either or both of the interstices and ends of the stent. Softening under pressure molds the balloon material such that it takes a permanent set into the stent. Once pressure is removed, the stent is interlocked with the surface of the balloon, providing substantially uniform contact between the balloon and the stent and a substantially uniform delivery profile.

[0011] As with the technique in the Jendersee patent, the technique in the Whelan patent has several drawbacks. Chemically softening the balloon material under pressure is expected to introduce inhomogeneities along the length of the balloon, such as varying wall thickness, which again may lead to failure of the balloon. Additionally, chemical alteration of the balloon, via application of a solvent to the surface of the balloon, may unpredictably degrade the mechanical characteristics of the balloon, thereby making accurate and controlled deployment of a stent difficult. Softening also adds cost, complexity, and time to the manufacturing process.

[0012] In view of the drawbacks associated with previously known methods and apparatus for loading a stent onto a stent delivery system, it would be desirable to provide methods and apparatus that overcome those drawbacks.

[0013] It would be desirable to provide methods and apparatus for loading a stent onto a stent delivery system that enhance positional stability of the stent during delivery.

[0014] It would further be desirable to provide methods and apparatus for loading a stent onto a stent delivery system wherein the delivery system comprises a crossing profile and flexibility suitable for use in tortuous and narrowed anatomy.

[0015] It would still further be desirable to provide methods and apparatus for loading a stent onto a stent delivery system that provide a substantially symmetrical expansion of the stent at deployment.

[0016] It would also be desirable to provide methods and apparatus for loading a stent onto a stent delivery system that do not unpredictably modify the mechanical characteristics of the balloon during fixation of the stent to the balloon.

[0017] In view of the foregoing, it is an object of the present invention to provide methods and apparatus for loading a stent onto a stent delivery system and deployment that overcome drawbacks associated with previously known methods and apparatus.

[0018] It is an object to provide methods and apparatus for loading a stent onto a stent delivery system that enhance positional stability of the stent during delivery.

[0019] It is an object to provide methods and apparatus for loading a stent onto a stent delivery system wherein the delivery system comprises a crossing profile and flexibility suitable for use in tortuous and narrowed anatomy.

[0020] It is also an object to provide methods and apparatus for loading a stent onto a stent delivery system that provide a substantially symmetrical expansion of the stent at deployment.

[0021] It is an object to provide methods and apparatus for loading a stent onto a stent delivery system that do not unpredictably modify the mechanical characteristics of the balloon during fixation of the stent to the balloon.

[0022] These and other objects of the present invention are achieved by providing methods and apparatus for cold-molding a stent to the balloon of a stent delivery system so that the balloon extends non-uniformly into the interstices of the stent. In a preferred embodiment, the stent is a balloon expandable stent and is manufactured in a fully-expanded state or in an intermediate-expanded state (i.e., having a diameter smaller than its fully-expanded, deployed diameter, but larger than its compressed delivery diameter).

[0023] The stent is disposed on the balloon of a delivery catheter, and the balloon and stent are placed within an elastic crimping tube. The balloon/stent/crimping tube assembly is then placed in a crimping tool, and the balloon is inflated, preferably only partially. The crimping tool is actuated to compress the stent on the outside of the partially inflated balloon and to cause creases of the balloon to extend non-uniformly into the interstices of the stent. Crimping occurs at a substantially constant temperature, without the use of chemicals. The balloon is then deflated, and the elastic crimping tube is removed.

[0024] Optionally, pillows or bumpers may be formed in the proximal and/or distal regions of the balloon during crimping that, in conjunction with the non-uniform creases of the balloon, prevent longitudinal movement of the stent with respect to the balloon during intravascular delivery.

[0025] Furthermore, one or more additional, secondary crimping steps may be performed to achieve a smoother delivery profile, in which a semi-rigid crimping tube is disposed over the stent delivery system, and the assembly is again disposed within the crimping tool. During secondary crimping, the crimping tool is actuated to further compress the stent onto the unpressurized balloon. Secondary crimping may alternatively be performed with the balloon partially or completely pressurized/inflated.

[0026] Apparatus of the present invention may be used with a variety of prior art stents, such as balloon expandable stents, and may include tubular slotted stents, connected stents, articulated stents, multiple connected or non-connected stents, and bistable stents. In addition to methods of production, methods of using

the apparatus of the present invention are provided.

[0027] Further features of the invention, its nature and various advantages will be more apparent from the following detailed description of the preferred embodiments, taken in conjunction with the accompanying drawings, in which like reference numerals refer to like parts throughout, and in which:

FIGS. 1A-1C are, respectively, a side view of a stent delivery system in accordance with the present invention, a cross-sectional view of the system along section line A--A in FIG. 1A, and a detail view of the balloon of the system non-uniformly extending within the interstices of the stent;

FIG. 2 is a flow chart showing the steps of the cold-molding process of the present invention;

FIGS. 3A-3C are, respectively, a side view of the distal end of the delivery catheter of the system of FIGS. 1 in an expanded configuration, and cross-sectional views of the catheter along section line B--B in FIG. 3A, showing the balloon evacuated to form radially extended wings and in a contracted configuration with the radially extended wings wrapped about the catheter;

FIGS. 4A-4C are, respectively, a side view, partially in section, of the wrapped delivery catheter of FIG. 3C having the stent of FIGS. 1 and an elastic crimping tube disposed thereover, the entire assembly disposed within a crimping tool; a cross-sectional view of the same along section line C--C in FIG. 4A; and a detail view of the expandable structure of the stent;

FIGS. 5A and 5B are, respectively, a cross-sectional view along section line C--C in FIG. 4A of the apparatus upon pressurization of the balloon, and a detail view of the expandable structure of the stent; FIG. 6 is a cross-sectional view along section line C--C in FIG. 4A during crimping after pressure has been removed;

FIG. 7 is a cross-sectional view along section line C--C in FIG. 4A of a possible configuration of the stent delivery system after crimping and removal of the elastic crimping tube;

FIG. 8 is a side view, partially in section, of the stent delivery system disposed within a semi-rigid crimping tube and within the crimping tool for optional secondary crimping; and

FIGS. 9A-9D are side views, partially in section, of the stent delivery system of FIGS. 1 disposed within a patient's vasculature, depicting a method of using the apparatus in accordance with the present invention.

[0028] The present invention comprises methods and apparatus for cold-molding a stent onto a stent delivery system. More specifically, the present invention provides methods and apparatus for obtaining a balloon having creases that extend non-uniformly into the inter-

stices of a stent loaded onto the exterior of the balloon, without the use of a heating or chemical process.

[0029] With reference to FIGS. 1, apparatus in accordance with the present invention is described. As seen in FIG. 1A, stent delivery system 10, illustratively shown in a collapsed delivery configuration, comprises balloon expandable stent 20 loaded on balloon 14 of delivery catheter 12. Stent 20 comprises an illustrative balloon expandable stent and may be replaced with other stents known in the art. As seen in FIGS. 1B and 1C, balloon 14 has creases 16 that extend non-uniformly into interstices 22 of stent 20.

[0030] In FIG. 1B, creases 16 are shown with varying slope and height about the circumference of stent delivery system 10. FIG. 1C depicts creases 16 as shaded areas and illustrates that creases 16 extend along the length of stent 20 within interstices 22. Line L indicates the longitudinal axis of stent 20 in FIG. 1C. It should be understood that creases 16 typically do not extend within every interstice 22 of stent 20.

[0031] Delivery catheter 12 preferably includes markers 17 disposed distal of and proximal to stent 20 that facilitate placement of stent 20 on balloon 14, and that facilitate positioning of stent delivery system 10 at a treatment site within a patient's vasculature. Markers 17 are preferably radiopaque and fabricated from a radiopaque material, such as platinum or gold. Catheter 12 preferably also comprises guide wire lumen 13 and inflation lumen 15, which is coupled to balloon 14. As described hereinbelow, during the cold-molding process of the present invention, proximal and/or distal pillows 19 optionally may be formed in balloon 14 during pressurized crimping. As with creases 16, pillows 19 act to reduce or prevent longitudinal movement of the stent on the balloon during intravascular delivery.

[0032] Balloon 14 is expandable by injection of a suitable medium, such as air or saline, via inflation lumen 15. Balloon 14 preferably expands stent 20 to a deployed configuration under application of pressure in the range of about 6-9 atm. Additionally, balloon 14 preferably has a rated burst pressure above 10 atm, and even more preferably between about 12-14 atm. Balloon 14 may be fabricated from a variety of materials, including Nylon, polyethylene terephthalate, polyethylene, and polyether/polyamide block copolymers, such as PEBAX.

[0033] Additionally, balloon 14 may be fabricated from an elastomeric polyester block copolymer having an aromatic polyester hard segment and an aliphatic polyester soft segment, such as "Pelprene," which is marketed by the Toyobo Corporation of Osaka, Japan. Balloon 14 also may be fabricated from a copolymer having a polybutylene terephthalate hard segment and a long chain of polyether glycol soft segment, such as "Hytrel" from the DuPont Corporation of Wilmington, DE.

[0034] Illustrative stent 20 may be fabricated from a variety of materials, including polymers and metals, and may comprise any of a variety of prior art stents, such as balloon expandable stents, including tubular slotted

stents, connected stents, articulated stents, multiple connected or non-connected stents, and bistable stents. Stent 20 also may include external coating C configured to retard restenosis or thrombus formation in the vessel region surrounding the stent. Alternatively, coating C may deliver therapeutic agents into the patient's blood stream or vessel wall.

[0035] Referring now to FIGS. 2-8, a method of producing stent delivery system 10 is described. FIG. 2 provides an overview of the cold-molding process of the present invention, while FIGS. 3-8 provide detailed views of these process steps.

[0036] As depicted in FIG. 2, the cold-molding process of the present invention involves steps of: obtaining a stent, step 102; obtaining a balloon catheter, step 103; disposing the stent on the balloon of the balloon catheter, step 104; and disposing an elastic crimping sleeve over the stent and balloon, step 105. In accordance with the method of the present invention, the balloon is then inflated- preferably only partially - with an inflatable medium, such as air, at step 106. The sleeve/stent/balloon assembly is then crimped within a crimping tool that compresses the stent onto the balloon, step 107, while the balloon is pressurized.

[0037] As described hereinbelow, this step causes the balloon to bulge into the interstices of the stent, and in addition, to form pillows 19, proximal of, and distal to, the ends of the stent to retain the stent in place during transluminal delivery. At step 108, the balloon is depressurized, and the elastic sleeve is removed to complete the stent loading process.

[0038] If desired, a semi-rigid sleeve optionally may be disposed over the stent/balloon assembly, and one or more additional crimping steps may be performed, steps 109 and 110 of FIG. 2.

[0039] Referring now to FIGS. 3-8, additional details of a preferred embodiment of the process of the present invention are illustrated and described. In FIGS. 3, balloon 14 of delivery catheter 12 preferably is folded prior to placement of stent 20 about balloon 14. Balloon 14 is first expanded, as in FIG. 3A, and then evacuated to form radially extended wings 18, as seen in FIG. 3B. Balloon 14 is illustratively depicted with four wings 18, but it should be understood that any number of wings may be provided, for example, two, three or five wings. In FIG. 3C, wings 18 are wrapped about the shaft of delivery catheter 12 to dispose catheter 12 in a contracted configuration. It should be understood that balloon 14 may alternatively be folded and/or disposed in a collapsed delivery configuration by other techniques, for example, with techniques that do not utilize wings.

[0040] With reference to FIGS. 4, stent 20 and elastic crimping tube 30 are disposed about balloon 14, preferably with stent 20 positioned between markers 17 of delivery catheter 12 (steps 102-105, FIG. 2). The balloon/stent/crimping tube assembly is inserted within crimping tool 40, as seen in FIG. 4A. Crimping tool 40 is preferably positioned between markers 17 to facilitate forma-

tion of optional pillows 19 during pressurization of balloon 14. Crimping tool 40 may be any of a variety of crimping tools known in the art. An illustrative crimping tool is described, for example, in U.S. Patent No. 6,082,990 to Jackson et al., which is incorporated herein by reference.

[0041] Referring to FIG. 4B, stent 20 may be directly placed about balloon 14, and elastic crimping tube 30 then may be loaded over the stent/balloon assembly. Alternatively, stent 20 may be placed within elastic crimping tube 30, and then the stent/tube assembly disposed surrounding balloon 14. As yet another alternative, crimping tube 30, or crimping tube 30 and stent 20, may be positioned within crimping tool 40; then, balloon 14, with or without stent 20 loaded thereon, may be positioned within crimping tool 40.

[0042] As depicted in FIG. 4C, stent 20 preferably is manufactured in an intermediate-expanded state having a diameter smaller than its expanded deployed diameter, but larger than its compressed delivery diameter, thereby facilitating positioning of stent 20 about balloon 14. When stent 20 is initially disposed surrounding balloon 14, the balloon does not substantially extend into interstices 22 of stent 20. It should be understood that stent 20 alternatively may be manufactured in a fully-expanded state.

[0043] In FIGS. 5, once stent 20 and crimping tube 30 are disposed about balloon 14 of delivery catheter 12, and once the entire assembly is disposed within crimping tool 40, balloon 14 is pressurized, for example, via an inflation medium delivered through inflation lumen 15 of catheter 12 (step 106, FIG. 2). Pressure application causes balloon 14 to enter a portion of interstices 22 of stent 20 in a non-uniform manner, as seen in the cross section of FIG. 5A and in the detail view of FIG. 5B. Crimping tube 30 and crimping tool 40 prevent expansion of stent 20 during partial or complete pressurization of balloon 14, as depicted in FIG. 5A.

[0044] The inflation medium is preferably delivered at a pressure in the range of about 6-8 atm. This pressure range is below the preferred rated burst pressure of balloon 14, which is above 10 atm, and even more preferably between about 12-14 atm, and thus ensures that the balloon does not puncture. The elasticity of crimping tube 30 allows the tube to expand slightly upon application of pressure, and to contract slightly during crimping. Tube 30 may be fabricated from any suitable elastic material, for example, a polymer, such as PEBAX. Elastic crimping tube 30 preferably has a hardness of between about 30 and 40 Shore Hardness, and more preferably a hardness of about 35 Shore Hardness.

[0045] With reference to FIG. 6, in conjunction with FIG. 4A, crimping tool 40 is actuated to crimp stent 20 onto balloon 14 (step 107, FIG. 2). Crimping tool 40 applies an inwardly-directed stress, σ_{crimp} , to the assembly. Initially, balloon 14 is still pressurized. Stent 20 is compressed onto the outside of balloon 14, causing the balloon to further bulge non-uniformly into interstices 22

of the stent. Crimping preferably proceeds along the length of the balloon/stent/tube assembly all at once but may alternatively proceed in sections, so that the assembly is gradually crimped along its length.

[0046] Balloon 14 is then depressurized, allowing crimping tool 40 to further compress stent 20 onto balloon 14, as seen in FIG. 6 (step 108, FIG. 2), which forms creases 16 of balloon 14 that extend non-uniformly within interstices 22 of the stent. Creases 16 are most clearly seen in FIGS. 1B and 1C. Optional pillows 19 of stent delivery system 10 are also formed. Since many prior art crimping tools 40 apply an inwardly-directed stress, σ_{crimp} , that is not uniform about the radius of balloon 14, elastic crimping tube 30 acts to more uniformly distribute the stress about the circumference of the balloon/stent assembly.

[0047] Stent delivery system 10 is removed from elastic crimping tube 30 and crimping tool 40 (step 108, FIG. 2). Stent delivery system 10 has a low-profile delivery configuration adapted for percutaneous delivery within a patient's vasculature, as described hereinbelow with respect to FIGS. 9. Creases 16, as well as pillows 19, secure stent 20 to balloon 14 between markers 17 of delivery catheter 12.

[0048] In contrast to prior art techniques described hereinabove, crimping in accordance with the present invention occurs at a substantially constant temperature, without the use of chemicals. In the context of the present invention, substantially constant temperature during crimping should be understood to include minor fluctuations in the actual temperature due to frictional losses, etc.

[0049] Importantly, the system of the present invention is not actively heated to thermally remodel the balloon, as described in U.S. Patent No. 5,836,965 to Jendryasek et al. Likewise, no solvents are added to soften and mold the balloon, as described in U.S. Patent No. 5,976,181 to Whelan et al. As described previously, both heating and solvents have significant potential drawbacks, including inhomogeneities along the length of the balloon, such as varying wall thickness. Varying wall thickness may yield areas of decreased strength that are susceptible to rupture upon inflation of the balloon during deployment of the stent. Additionally, heating and cooling, as well as addition of solvents, increases the complexity, time, and cost associated with affixing the stent to the balloon.

[0050] Theoretical bounds for the radial stress that may be applied to balloon 14 during crimping, while the balloon is pressurized, may be estimated by modeling balloon 14 as an idealized tube and assuming crimping tool 40 applies an evenly distributed, inwardly-directed radial stress, σ_{crimp} . Stent 20 and elastic crimping tool 30, meanwhile, theoretically resist the crimping stress with an outwardly-directed radial stress, $\sigma_{\text{resistance}}$. Thus, the composite inwardly-directed radial stress, σ_{in} , applied to balloon 14 may be idealized as:

$$\sigma_{\text{in}} = \sigma_{\text{crimp}} - \sigma_{\text{resistance}} \quad (1)$$

Pressurization/inflation of balloon 14 similarly may be modeled as an evenly distributed, outwardly-directed radial stress, σ_{out} , and it may be assumed that the rated burst pressure of balloon 14 is the yield stress of the balloon, σ_y . A stress balance provides:

$$\sigma_{\text{in}} - \sigma_{\text{out}} < \sigma_y \quad (2)$$

Thus, a theoretical upper bound for the radial stress, σ_{in} , that may be applied to balloon 14 is:

$$\sigma_{\text{in}} < \sigma_y + \sigma_{\text{out}} \quad (3)$$

A theoretical lower bound for σ_{in} also may be found by observing that, in order to compress stent 20 onto the exterior of balloon 14, crimping tool 40 must apply a radial stress, σ_{crimp} , that is greater than the net stress provided by resistance of stent 20 and crimping tube 30, $\sigma_{\text{resistance}}$, and by the inflation of balloon 14, σ_{out} :

$$\sigma_{\text{crimp}} > \sigma_{\text{out}} + \sigma_{\text{resistance}} \quad (4)$$

Combining Equation (1) and (4) provides a lower bound for σ_{in} :

$$\sigma_{\text{in}} > \sigma_{\text{out}} \quad (5)$$

Finally, combining Equations (3) and (5) provides a range for σ_{in} :

$$\sigma_{\text{out}} < \sigma_{\text{in}} < \sigma_y + \sigma_{\text{out}} \quad (6)$$

[0051] As an example, assuming a burst pressure, σ_y , of 12 atm and a balloon pressurization, σ_{out} , of 8 atm, the balloon will theoretically withstand an inwardly-directed stress, σ_{in} , of up to 20 atm. Furthermore, in order to ensure that stent 20 is crimped onto balloon 14, σ_{in} must be greater than 8 atm. Thus, the inwardly-directed radial stress must be between 8 and 20 atm. Assuming, for example, a resistance stress, $\sigma_{\text{resistance}}$, of 2 atm, crimping tool 40 must apply a crimping stress, σ_{crimp} , between 10 and 22 atm. As one of ordinary skill will readily understand, the actual radial stress applied should be further optimized within this range to provide a safety factor, optimal crimping, etc. Since balloon 14 is not in reality an idealized tube, stresses applied to the balloon will have a longitudinal component in addition to the radial component, which may be, for example, accounted for in the safety factor.

[0052] With reference now to FIG. 7, a possible configuration of the stent delivery system after crimping and removal of elastic crimping tube 30 is described. One or more struts 21 of stent 20 may be incompletely compressed against balloon 14. Such a strut may potentially snag against the patient's vasculature during delivery, and thereby prevent positioning of stent delivery system 10 at a treatment site. Additionally, pressurized crimping may result in a delivery profile for delivery system 10 that is more polygonal than cylindrical, thereby applying undesirable stresses on the vessel wall during transluminal insertion. Accordingly, it may be desirable to perform an optional secondary crimping step after balloon 14 has been depressurized.

[0053] Referring to FIG. 8, in order to reduce the potential for incompletely compressed individual struts 21 of stent 20, and to provide a more uniform cylindrical delivery profile, one or more additional, secondary crimping steps may be performed on stent delivery system 10. In FIG. 8, stent delivery system 10 is disposed within semi-rigid crimping tube 50, which is disposed within crimping tool 40 (step 109, FIG. 2). Tube 50 may be fabricated from any suitable semi-rigid material. As with elastic crimping tube 30, semi-rigid crimping tube 50 preferably comprises a polymer, such as PEBAX. Semi-rigid crimping tube 50 preferably has a hardness of between about 50 and 60 Shore Hardness, and more preferably a hardness of about 55 Shore Hardness.

[0054] With stent delivery system 10 disposed within semi-rigid tube 50 and crimping tool 40, tool 40 is actuated to compress individual struts 21 against balloon 14 and to give delivery system 10 the substantially cylindrical delivery profile of FIG. 1B (step 110, FIG. 2). As with elastic crimping tube 30, semi-rigid tube 50 acts to evenly distribute crimping stresses applied by crimping tool 40 around the circumference of the stent/balloon assembly. Since balloon 14 is not pressurized, secondary crimping preferably proceeds in sections along the length of stent delivery system 10. However, as will be apparent to those of skill in the art, secondary crimping may proceed in one step. Optionally, balloon 14 may be pressurized during secondary crimping.

[0055] Referring now to FIGS. 9, a method of using stent delivery system 10 of the present invention is described. Stent delivery system 10 is disposed in a contracted delivery configuration with stent 20 disposed over balloon 14 of delivery catheter 12. Creases 16 of balloon 14 non-uniformly extend within interstices 22 of stent 20. Creases 16, in conjunction with optional pillows 19, act to secure stent 20 to balloon 14. As seen in FIG. 9A, the distal end of catheter 12 is delivered to a target site T within a patient's vessel V using, for example, well-known percutaneous techniques. Target site T may, for example, comprise a stenosed region of vessel V. The radiopacity of markers 17 may facilitate positioning of system 10 at the target site. Alternatively, stent 20 or other portions of catheter 12 may be radiopaque to facilitate positioning.

[0056] In FIG. 9B, balloon 14 is inflated, for example, via an inflation medium delivered through inflation lumen 15 of catheter 12. Stent 20 expands to the deployed configuration in which it contacts the wall of vessel V at target site T. Expansion of stent 20 opens interstices 22 of the stent and removes the non-uniform creases of balloon 14 from within the interstices. Additionally, stent 20 has a diameter in the deployed configuration that is larger than the diameter of optional pillows 19, thereby facilitating removal of stent 20 from delivery catheter 12. Balloon 14 is then deflated, as seen in FIG. 9C, and delivery catheter 12 is removed from vessel V, as seen in FIG. 9D.

[0057] Stent 20 remains in place within vessel V in the deployed configuration in order to reduce restenosis and recoil of the vessel. Stent 20 also may comprise external coating C configured to retard restenosis or thrombus formation around the stent. Alternatively, coating C may deliver therapeutic agents into the patient's blood stream or a portion of the vessel wall adjacent to the stent.

[0058] Although preferred illustrative embodiments of the present invention are described hereinabove, it will be evident to those skilled in the art that various changes and modifications may be made therein without departing from the invention.

[0059] For example, stent delivery system 10 may be produced without using elastic crimping tube 30. In this case, the stent/balloon assembly would be loaded directly into crimping tool 40, which would limit expansion of balloon 14 during pressurization. Likewise, semi-rigid crimping tube 50 may be eliminated from the secondary crimping procedure. If crimping tubes are not used, crimping tool 40 preferably applies an inwardly-directed stress that is substantially evenly distributed about the circumference of the stent/balloon assembly.

[0060] Additionally, balloon 14 may be depressurized prior to crimping stent 20 onto the balloon. This may be particularly beneficial when crimping long stents, for example, stents longer than about 50 mm. Pressurization of balloon 14 may cause the balloon to increase in longitudinal length. When crimping a long stent 20 onto a correspondingly long balloon 14, this increase in balloon length is expected to be more significant, for example, greater than about 1 mm.

[0061] If stent 20 is crimped onto balloon 14 while the balloon is pressured, significant stresses may be encountered along creases 16 after balloon 14 is depressurized, due to contraction of the balloon back to its shorter, un-inflated longitudinal length. These stresses may, in turn, lead to pinhole perforations of balloon 14. Thus, since pressurization of balloon 14 causes the balloon to extend at least partially within interstices 22 of stent 20 in a non-uniform manner, as seen in FIG. 5A, it is expected that crimping after depressurization will still establish creases 16 of stent delivery system 10, in accordance with the present invention. Obviously, crimping after depressurization may be done with stents

20 of any length, not just long stents.

Claims

1. A stent delivery system having a contracted delivery configuration and an expanded deployed configuration, the stent delivery system comprising:
 - a stent; and
 - a delivery catheter having an inflatable balloon, the stent disposed about the balloon, wherein the balloon comprises creases that extend non-uniformly within interstices of the stent in the contracted delivery configuration.
2. The stent delivery system of claim 1, wherein the inflatable balloon further comprises pillows disposed proximally and distally of the stent in the contracted delivery configuration.
3. The stent delivery system of claim 1 or 2, wherein the delivery catheter further comprises markers.
4. The stent delivery system of claim 3, wherein the markers are radiopaque.
5. The stent delivery system of claim 1, 2, 3 or 4, wherein the stent comprises an external coating.
6. The stent delivery system of claim 5, wherein the coating is configured to retard restenosis or thrombus formation around the stent.
7. The stent delivery system of claim 5 or 6, wherein the coating is configured to deliver therapeutic agents into a patient's blood stream or vessel wall when implanted within the patient's vasculature.
8. A method of fabricating a stent delivery system comprising:
 - providing apparatus comprising a stent and a delivery catheter having an inflatable balloon; disposing the stent about the inflatable balloon; placing the balloon and stent within a crimping tool; inflating the balloon; actuating the crimping tool to compress the stent on the outside of the balloon at a substantially constant temperature, thereby causing the balloon to extend non-uniformly into interstices of the stent; and
 - deflating the balloon while the crimping tool is still actuated, thereby securing non-uniform creases of the balloon within the interstices of the stent and forming the stent delivery system.
9. The method of claim 8 further comprising removing the stent delivery system from the crimping tool.
10. The method of claim 8 or 9, wherein in deflating the balloon further comprises forming proximal and/or distal pillows.
11. The method of claim 8, 9 or 10, comprising performing secondary crimping.
12. The method of claim 11, wherein secondary crimping comprises:
 - de-actuating the crimping tool; and
 - re-actuating the crimping tool to further compress the stent on the outside of the balloon.
13. The method of claim 12 further comprising de-actuating the crimping tool.
14. The method of any one of claims 8 to 13, wherein inflating the balloon further comprises partially inflating the balloon.
15. A method of fabricating a stent delivery system comprising:
 - providing apparatus comprising a stent and a delivery catheter having an inflatable balloon; disposing the stent about the inflatable balloon; placing an elastic crimping tube over the stent and balloon; placing the balloon, stent, and elastic crimping tube within a crimping tool; inflating the balloon; actuating the crimping tool to compress the stent on the outside of the balloon at a substantially constant temperature, thereby causing the balloon to extend non-uniformly into interstices of the stent; and
 - deflating the balloon while the crimping tool is still activated, thereby securing non-uniform creases of the balloon within the interstices of the stent and forming the stent delivery system.
16. The method of claim 15 further comprising de-actuating the crimping tool and removing the stent delivery system from the elastic crimping tube.
17. The method of claim 15 or 16, wherein deflating the balloon further comprises forming proximal and/or distal pillows.
18. The method of claim 15, 16 or 17, further comprising performing secondary crimping.
19. The method of claim 18, wherein secondary crimping comprises:

placing a semi-rigid crimping tube over the stent delivery system;
 placing the stent delivery system and semi-rigid crimping tube within the crimping tool; and
 re-actuating the crimping tool to further compress the stent on the outside of the balloon. 5

deflating the balloon; and
 removing the delivery catheter from the patient's vessel.

20. The method of claim 19 further comprising de-actuating the crimping tool and removing the stent delivery system from the semi-rigid crimping tube. 10

21. The method of claim 19 or 20, wherein re-actuating the crimping tool comprises actuating the crimping tool in sections along a length of the stent delivery system. 15

22. The method of any one of claims 15 to 21, wherein inflating the balloon further comprises partially inflating the balloon. 20

23. A method of fabricating a stent delivery system comprising:

providing apparatus comprising a stent and a delivery catheter having an inflatable balloon; 25
 disposing the stent about the inflatable balloon;
 placing the balloon and stent within a crimping tool;
 inflating the balloon;
 deflating the balloon; and 30
 actuating the crimping tool to compress the stent on the outside of the balloon at a substantially constant temperature, thereby securing non-uniform creases of the balloon within the interstices of the stent and forming the stent delivery system. 35

24. A method for stenting at a target site within a patient's vessel, the method comprising: 40

providing a stent delivery system comprising a stent and a delivery catheter with an inflatable balloon, the stent disposed about the inflatable balloon, wherein the balloon has creases that extend non-uniformly within interstices of the stent; 45
 percutaneously delivering the stent delivery system to the target site within the patient's vessel in a contracted delivery configuration; and
 expanding the stent delivery system to an expanded deployed configuration, wherein the balloon is inflated, the interstices of the stent open, removing the creases of the balloon from the interstices, and the stent engages the target site. 55

25. The method of claim 24 further comprising:

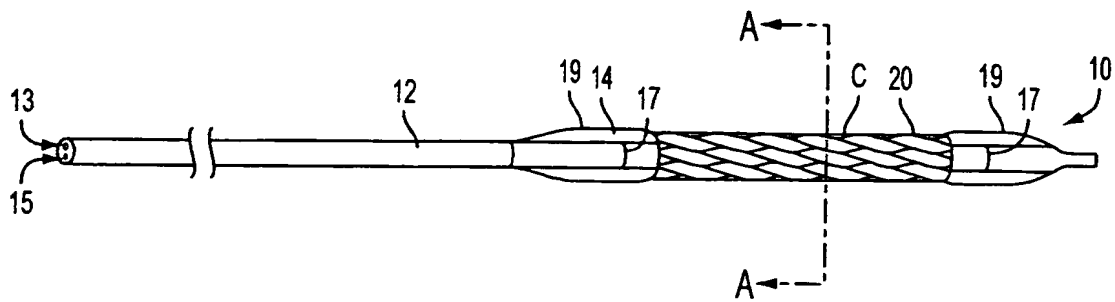


FIG. 1A

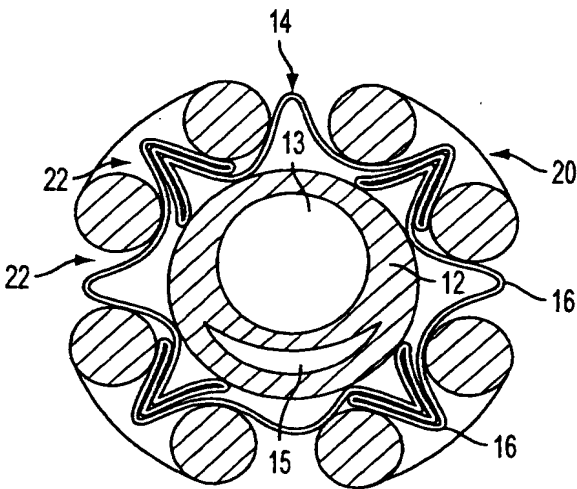


FIG. 1B

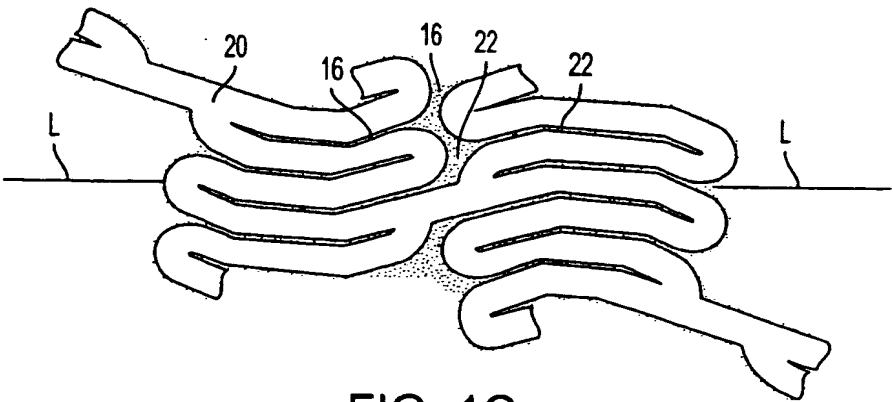


FIG. 1C

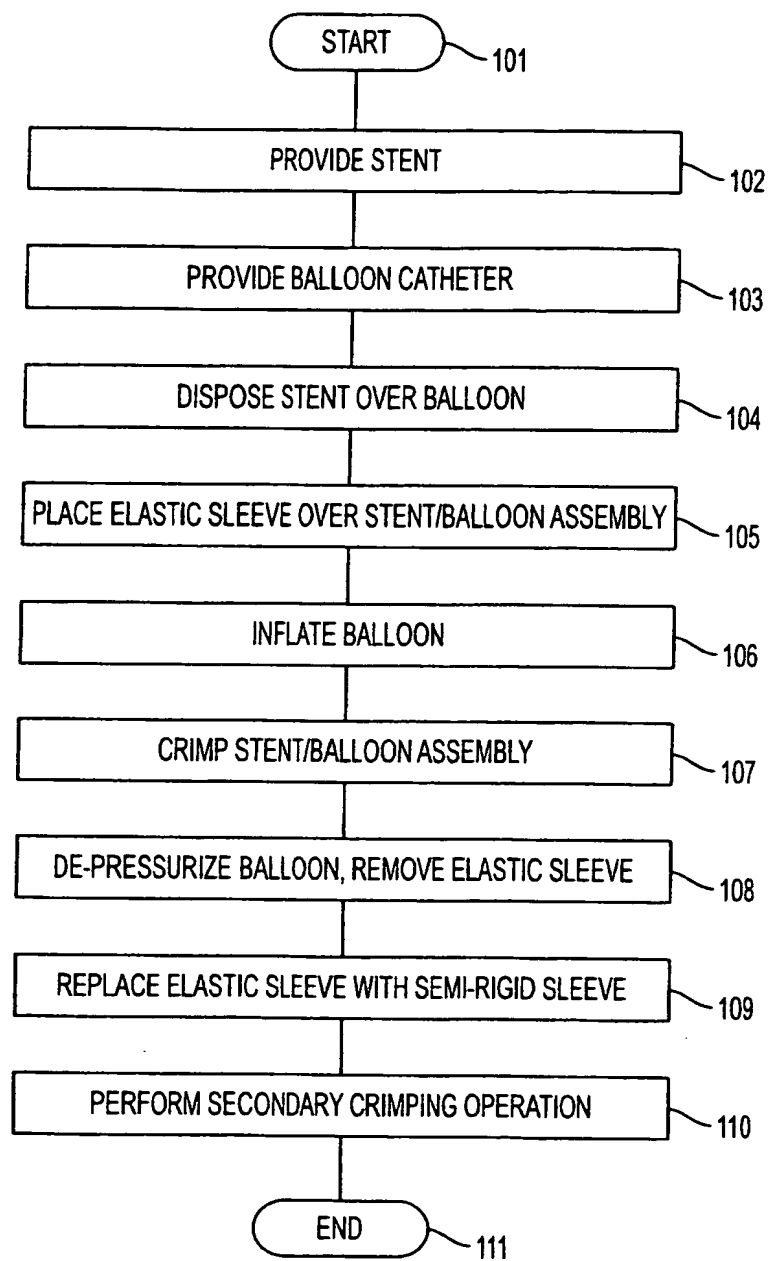


FIG. 2

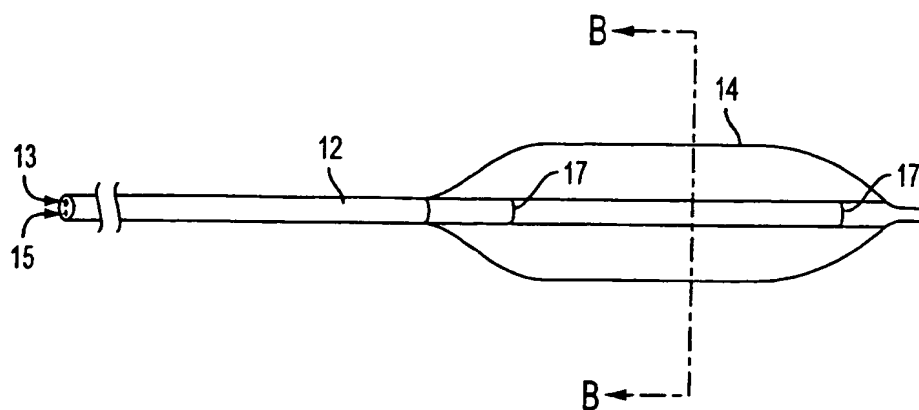


FIG. 3A

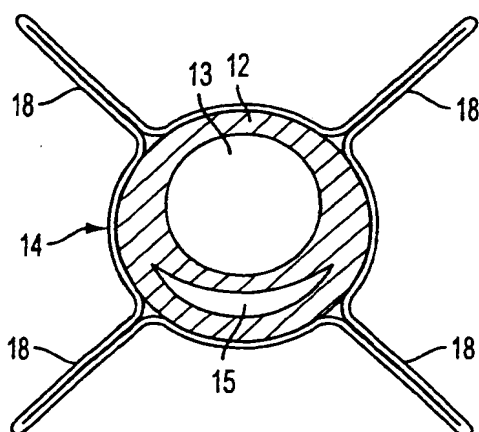


FIG. 3B

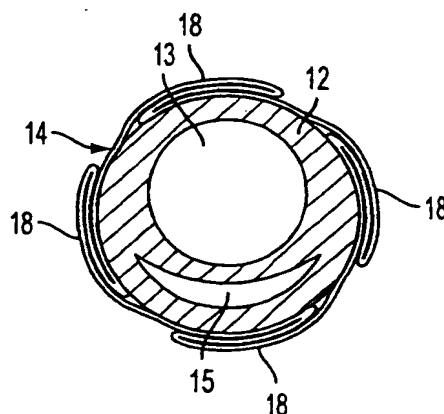


FIG. 3C

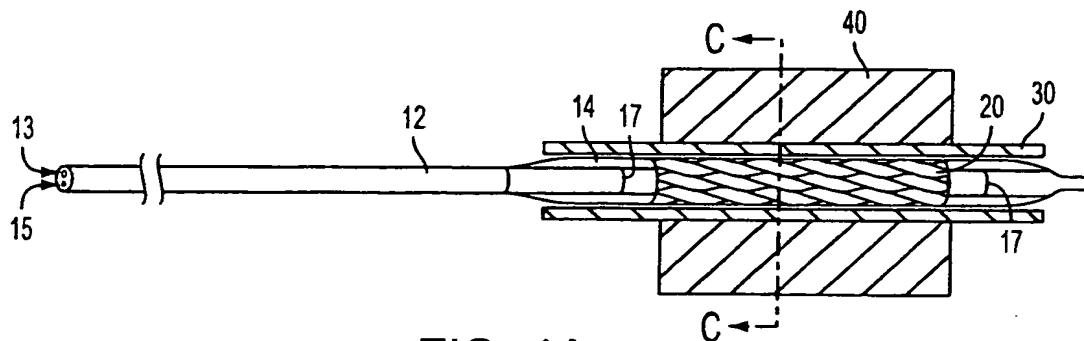


FIG. 4A

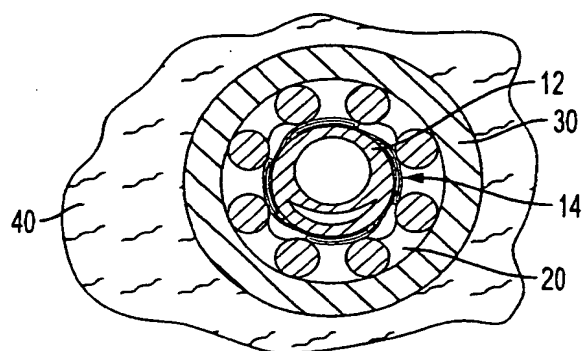


FIG. 4B

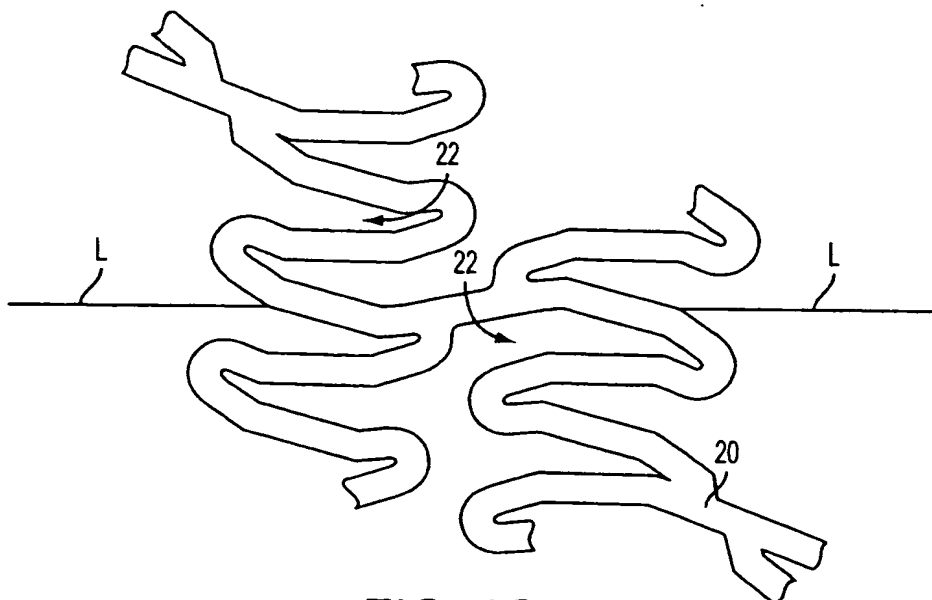


FIG. 4C

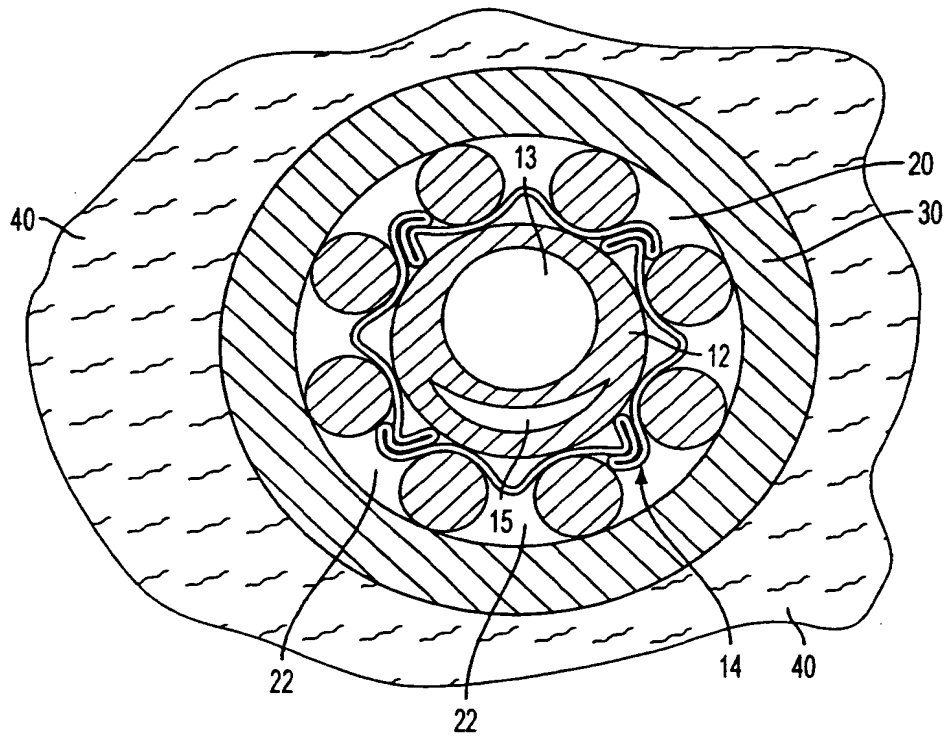


FIG. 5A

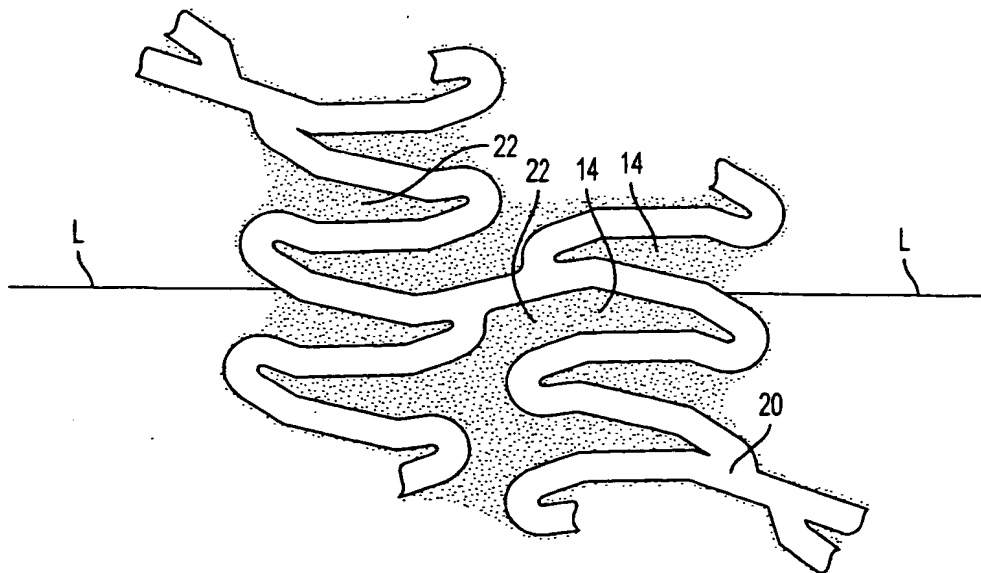


FIG. 5B

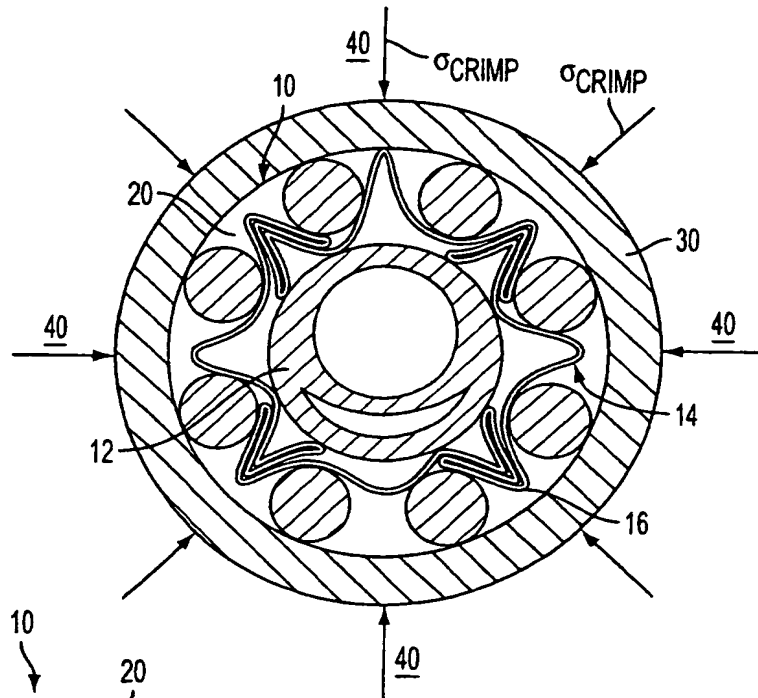


FIG. 6

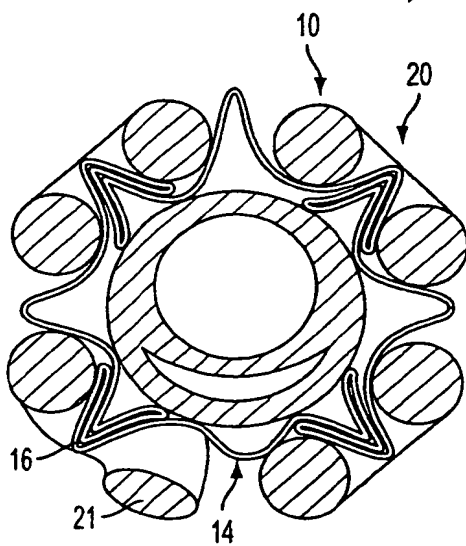


FIG. 7

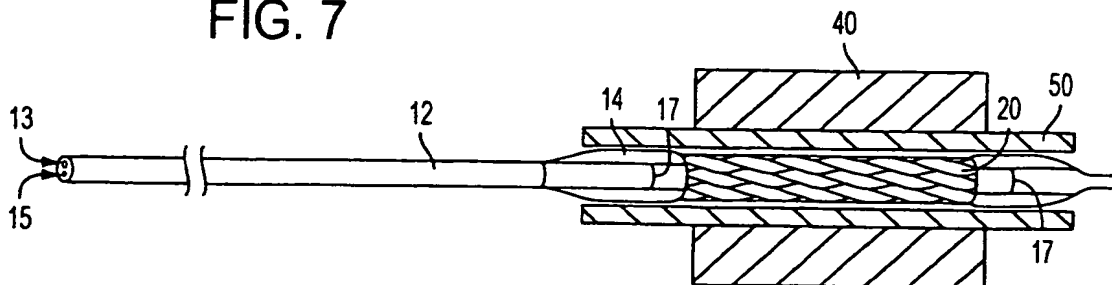


FIG. 8

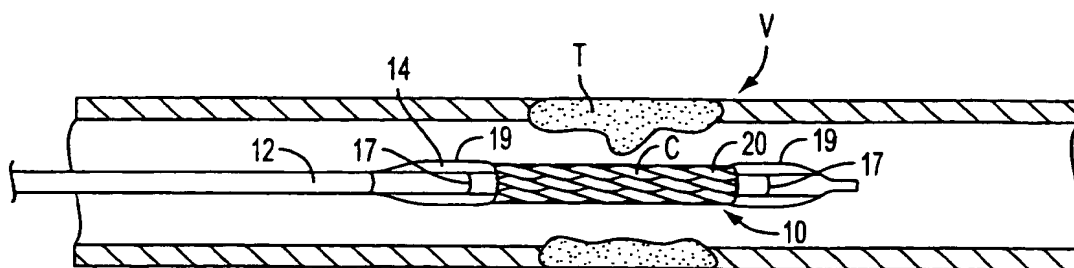


FIG. 9A

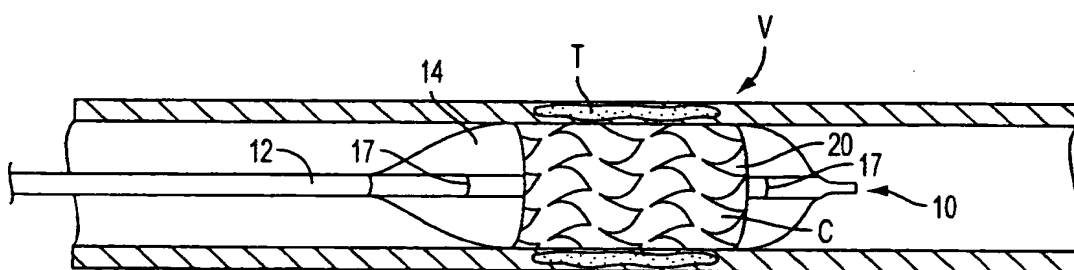


FIG. 9B

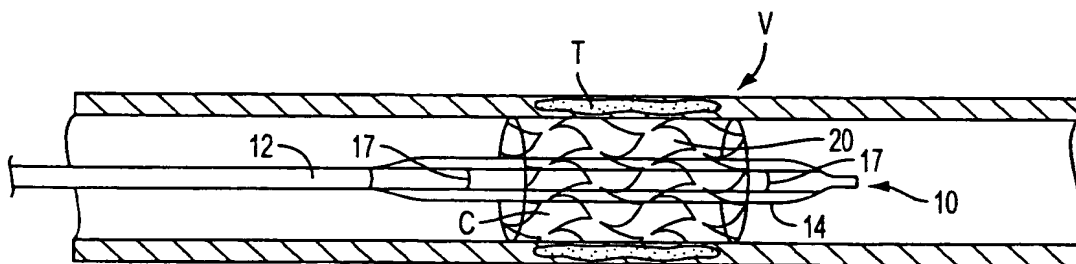


FIG. 9C


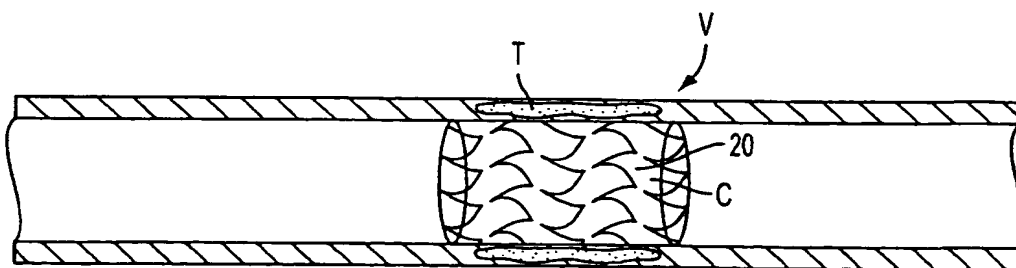


FIG. 9D



Eur päisch s Patentamt
Eur p an Patent Office
Offic européen d s br vets



(11) **EP 1 295 570 A3**

(12) **EUROPEAN PATENT APPLICATION**

(88) Date of publication A3:
03.03.2004 Bulletin 2004/10

(51) Int Cl.7: **A61F 2/00, A61F 2/06**

(43) Date of publication A2:
26.03.2003 Bulletin 2003/13

(21) Application number: **02018239.0**

(22) Date of filing: **21.08.2002**

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
IE IT LI LU MC NL PT SE SK TR**
Designated Extension States:
AL LT LV MK RO SI

(72) Inventors:
• **Schwager, Michael**
8404 Winterthur (CH)
• **Frei, Martin**
8200 Schaffhausen (CH)
• **Ha, Suk-Woo**
8246 Langwiesen (CH)

(30) Priority: **19.09.2001 US 957216**

(71) Applicant: **Abbott Laboratories Vascular
Enterprises Limited**
Dublin 2 (IE)

(74) Representative: **VOSSIUS & PARTNER**
Siebertstrasse 4
81675 München (DE)

(54) **Cold-molding process for loading a stent onto a stent delivery system**

(57) A method of making a stent delivery system is provided in which a delivery catheter has a balloon that extends non-uniformly into interstices of a stent. In accordance with the method a balloon/stent/crimping tube assembly is placed in a crimping tool, the balloon is inflated, and the crimping tool is actuated to compress the stent on the outside of the balloon without application of

heat or chemicals, thereby causing creases of the balloon to extend non-uniformly into the interstices of the stent. Optionally, pillows may be formed in the balloon to prevent longitudinal movement of the stent with respect to the balloon during intravascular delivery. One or more secondary crimpings also may be performed to achieve a smoother delivery profile.

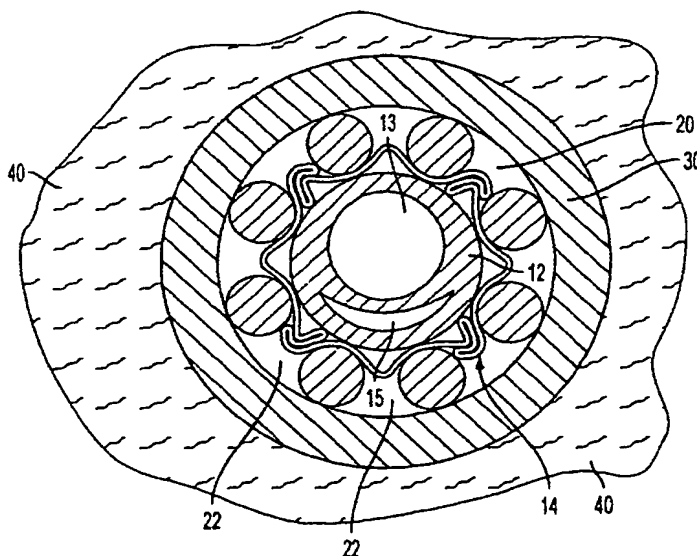


FIG. 5A



European Patent
Office

PARTIAL EUROPEAN SEARCH REPORT

Application Number

which under Rule 45 of the European Patent Convention shall be considered, for the purposes of subsequent proceedings, as the European search report

EP 02 01 8239

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
X,D	US 5 836 965 A (JENDERSEE BRAD ET AL) 17 November 1998 (1998-11-17)	1-4	A61F2/00 A61F2/06
Y	* column 5, line 14 - column 8, line 13 * * figures 1,6 *	5-7	
X,D	US 5 976 181 A (WHELAN SEAN ET AL) 2 November 1999 (1999-11-02)	1-4	
Y	* column 3, line 66 - column 6, line 36 * * figures 1,7 *	5-7	
Y	EP 0 716 836 A (ADVANCED CARDIOVASCULAR SYSTEM) 19 June 1996 (1996-06-19) * page 1, line 15 - page 9, line 28 *	5-7	
			TECHNICAL FIELDS SEARCHED (Int.Cl.7)
			A61F
INCOMPLETE SEARCH			
<p>The Search Division considers that the present application, or one or more of its claims, does/do not comply with the EPC to such an extent that a meaningful search into the state of the art cannot be carried out, or can only be carried out partially, for these claims.</p> <p>Claims searched completely :</p> <p>Claims searched incompletely :</p> <p>Claims not searched :</p> <p>Reason for the limitation of the search: see sheet C</p>			
Place of search Munich		Date of completion of the search 17 October 2003	Examiner Skorovs, P
<p>CATEGORY OF CITED DOCUMENTS</p> <p>X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document</p> <p>T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons</p> <p>& : member of the same patent family, corresponding document</p>			

EPO FORM 1503 03.82 (P04C07)



European Patent
Office

INCOMPLETE SEARCH
SHEET C

Application Number
EP 02 01 8239

Claim(s) searched completely:
1-7

Claim(s) not searched:
24, 25

Reason for the limitation of the search (non-patentable invention(s)):

Article 52 (4) EPC - Method for treatment of the human or animal body by surgery



European Patent
Office

Application Number
EP 02 01 8239

CLAIMS INCURRING FEES

The present European patent application comprised at the time of filing more than ten claims.

☒ Only part of the claims have been paid within the prescribed time limit. The present European search report has been drawn up for the first ten claims and for those claims for which claims fees have been paid, namely claim(s):

☐ No claims fees have been paid within the prescribed time limit. The present European search report has been drawn up for the first ten claims.

LACK OF UNITY OF INVENTION

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

see sheet B

☐ All further search fees have been paid within the fixed time limit. The present European search report has been drawn up for all claims.

☐ As all searchable claims could be searched without effort justifying an additional fee, the Search Division did not invite payment of any additional fee.

☐ Only part of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the inventions in respect of which search fees have been paid, namely claims:

☒ None of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the invention first mentioned in the claims, namely claims:

1-7



European Patent
Office

LACK OF UNITY OF INVENTION
SHEET B

Application Number

EP 02 01 8239

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

1. claims: 1-7

A stent delivery system comprising: a stent; a delivery catheter having an inflatable balloon, the stent disposed about the balloon, wherein the balloon comprises creases that extend non-uniformly within interstices of the stent.

2. claims: 8-23

A method of fabricating a stent delivery system comprising: disposing the stent about the inflatable balloon; placing the balloon and the stent within a crimping tool; and actuating the crimping tool to compress the stent on the outside of the balloon at the substantially constant temperature, thereby securing non-uniform creases of the balloon within the interstices of the stent.

ANNEX TO THE EUROPEAN SEARCH REPORT ON EUROPEAN PATENT APPLICATION NO.

EP 02 01 8239

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

17-10-2003

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 5836965	A	17-11-1998	AT 221399 T	15-08-2002
			AU 708433 B2	05-08-1999
			AU 3957195 A	15-05-1996
			CA 2202257 A1	02-05-1996
			DE 69527636 D1	05-09-2002
			DE 69527636 T2	03-04-2003
			EP 0787020 A1	06-08-1997
			JP 8164210 A	25-06-1996
			WO 9612517 A1	02-05-1996
			US 6309402 B1	30-10-2001
			US 6159229 A	12-12-2000
US 5976181	A	02-11-1999	AU 9093098 A	12-04-1999
			WO 9915106 A1	01-04-1999
EP 0716836	A	19-06-1996	US 5637113 A	10-06-1997
			AU 4031295 A	20-06-1996
			CA 2164684 A1	14-06-1996
			DE 69521592 D1	09-08-2001
			DE 69521592 T2	25-10-2001
			EP 1084721 A2	21-03-2001
			EP 0716836 A1	19-06-1996
			JP 3231607 B2	26-11-2001
			JP 8224297 A	03-09-1996
			NZ 331390 A	28-02-2000
			US 5700286 A	23-12-1997

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82